



Investigating Some Properties of Nanocomposites for Dental Restoration Materials

¹Israa F. Ghazi*, ¹Jawad K. Oleiwi, ²Sihama I. Salih, ³Mohammed A. Mutar

¹Materials Engineering Department, University of Technology – Iraq

²Anesthesia Techniques Department, Hilla University College – Iraq

³Chemical Engineering Departments, College of Engineering, University of AL-Qadisiyah – Iraq

Article information

Article history:

Received: January, 14, 2022

Accepted: March, 28, 2022

Available online: December, 10, 2022

Keywords:

Dental Composites,
Resin-Based Composites,
Wear Resistance,
Hardness,
Surface Roughness

*Corresponding Author:

Israa. F. Ghazi

israa.ghazi@qu.edu.iq

Abstract

In this work, it was evaluated the wear resistance, hardness, and surface roughness values of resin-based composites that applied in dentistry as restorative materials. The resin composites were made from six types of resin matrixes (A, B, C, D, E, and F) and each one of them has contained different types and ratios of monomers as well as the inorganic nano-fillers (SiO₂, ZrO₂, HA, and Al₂O₃). For each test, thirty specimens were prepared, which were classified into six groups depending on the types of the resin matrix and fillers used in the composites. The results prove that the nanocomposites that have the lowest rate of wear were the group E which was derived from the resin matrix of the group E that has monomers are (BIS-GMA, meth acrylamide, methacrylic acid, and 1-6 hexanediol methacrylate) with values range from 8.11 to 6.11 mm³/mm depending on the filler type material. All prepared composites resin materials (A to F) showed an increase in their hardness values as regards the reference, group D showed the highest hardness value followed by group B while group C was the lowest. The highest mean roughness was shown in groups A and F with 0.82 and 0.79 μm respectively, while the smoother surfaces among all groups were groups B and D which had significantly fewer roughness values of 0.16 and 0.19 μm respectively.

DOI: [10.53293/jasn.2022.4629.1131](https://doi.org/10.53293/jasn.2022.4629.1131), Department of Applied Sciences, University of Technology

This is an open access article under the CC BY 4.0 License.

1. Introduction

Due to their good esthetics, resin composites have recently become the most widely used materials in restorative dentistry and are made up of a polymer resin matrix, nanofillers materials as reinforcement, and coupling agents (Silane). Wear resistance is a critical factor to decide the life expectancy of the resin composites, among other mechanical properties [1-4]. During mastication, direct contact is present between the teeth with the restorations, oral parafunction, abrasive particles in brushing tooth, and chemical effects generated by food components all contribute to the deterioration of restoration materials used in the oral environment [5]. This will result in a lack of sufficient wear resistance [6]. In the oral environment, predicting the wear behavior of restorative materials is an essential clinical challenge, high wear can cause loss of the support of a posterior tooth, failure of vertical

dimension of occlusion, reduce the efficiency of masticatory, and fatigue of masticatory muscles. The restoration not only should appear good when it has installed, but also it should look good over time. Abrasive substances abrade the resin matrix and expose fillers in many circumstances, potentially increasing the roughness of composite restorations surface. The surface roughness can cause the building up of bacterial biofilm a major cause of gingival irritation leads to a rise in the risk of secondary caries [7]. Therefore, it must be mentioned the good surface characteristics of a resin composite provide the clinical longevity of a restoration [8]. As a result, the wear of composite restorative materials is identified to be dependent on the characteristics of reinforcement particles, specifically the amount and size of those particles, [9] as well as the resin composition [10]. Nano filler particles reduced the interparticle gap, resulting in less wear [11]. Effects of adhesive through two touched surfaces, fatigue, abrasion, and corrosive effects are all fundamental processes that act in different combinations depending on the qualities of the materials. The principal clinical wear mechanisms for dental resin composites have long been assumed to be abrasion and attrition [12]. Hardness is another significant metric for determining a restorative material's mechanical strength and resistance to intra-oral softening [13]. It was used to predict the material's wear behavior. It also has something to do with the ease of finishing and polishing. The relationship between a material's hardness and its wear resistance is a point of contention. [14]. The variation of hardness values between all composite restoratives surfaces can clarify the variation in the rate of wear. Consequently, it found that the wear of restorative materials is determined by some factors, especially the hardness of the restorative material [15]. Both the surface roughness value and wear affected the strength of the resultant composites that was increased with a decrease of surface roughness and has significant differences for the same surface roughness values with different directions of scratch [16]. From what was mentioned about the importance of the surface characteristics of the durability of a resin composite as clinical restoration, this study aimed to evaluate the wear resistance, hardness, and surface roughness (Ra) of prepared resin composites based on copolymer matrix to use as restorative materials.

2. Materials and Methods

2.1 Materials

The main used materials are BIS-GMA (40%) as a major monomer and 1-6 hexanediol methacrylate (20%) as crosslinked supplied by Sigma Aldrich/USA Company and other monomers are listed in Table 1. Six groups of resins were used for the production of dental composites; each matrix was prepared from four monomers named to the group of matrix monomers (A, B, C, D, E, and F).

Table 1: Monomers, and their added ratios for each group of the prepared matrices resins.

Groups	Monomers	Adding Ratio %	Supplier
A	1. 2-ethylhexylmethacrylate	20	MERCK/Germany
	2. methylmethacrylate	20	MERCK/Germany
B	1. methacrylic acid	20	MERCK/Germany
	2. methacrylate	20	MERCK/Germany
C	1. methacrylic acid	20	MERCK/Germany
	2. polyethylene glycol 3500	20	MERCK/Germany
D	1. methacrylamide	20	MERCK/Germany
	2. methacrylic acid	20	MERCK/Germany
E	1. 2-ethylhexylmethacrylate	20	Aldrich/USA
	2. polyethylglycol	10	Aldrich/USA
	3. bisphenoladimethacrylate	10	Aldrich/USA
F	1. methacryate	20	MERCK/Germany
	2. polyethylene glycol	20	Aldrich/USA

Each group was reinforced by different types of inorganic nanoparticles listed in Table 2. For each test, 30 specimens consisting of 5 specimens of every prepared composite one for unreinforced polymer and 4 for each type of the used fillers. Preparation copolymeric matrices and their nanocomposite was achieved under continuous N₂ gas flow as shown in Figure 1, the components of every group of monomers listed in Table 1, were mixed for about 90 minutes, using N₂ is to assist in removing dissolved oxygen. Then 0.4 gm of zinc oxide as an

antibacterial agent, (0.5wt %) accelerator material (DMAEMA) and 0.5wt% of camphor quinine as an initiator, were used with continuous mixing for another 20 minutes to produce matrices as a copolymer. To prepare the nanocomposites, nano-fillers (ZrO_2 , SiO_2 , HA, and Al_2O_3) with (2wt %) ratio, were added individually for each set of the matrix monomers mention former in Table 1. Then the same procedures used when preparing the matrices of copolymers were followed. Afterward, each of the prepared specimens was photo-cured and radiated in different positions for 60 s using an instrument of light curing (Elipar Free light 2LED, 3 M ESPE) at the intensity of 1500 mW/cm^2 . After polymerization and previous to performing any mechanical tests, the entire specimen was kept for 48h in distilled water at 37°C and 100% humidity.

Table 2: Nano-fillers and their particle sizes, the supplier company used in prepared composites.

Filler Type	Particles Size (nm)	Purity%	Supplier Company
Zirconium Oxide	30-40	99.9	Skyspring Nanomaterials
Silicon Oxide	10-20	99.0	Skyspring Nanomaterials
HydroxyApatite	25	97.0	Hualanchem.Co.China
Aluminum Oxide	20-40	99.0	Skyspring Nanomaterials
Zinc Oxide		99.0	GCC

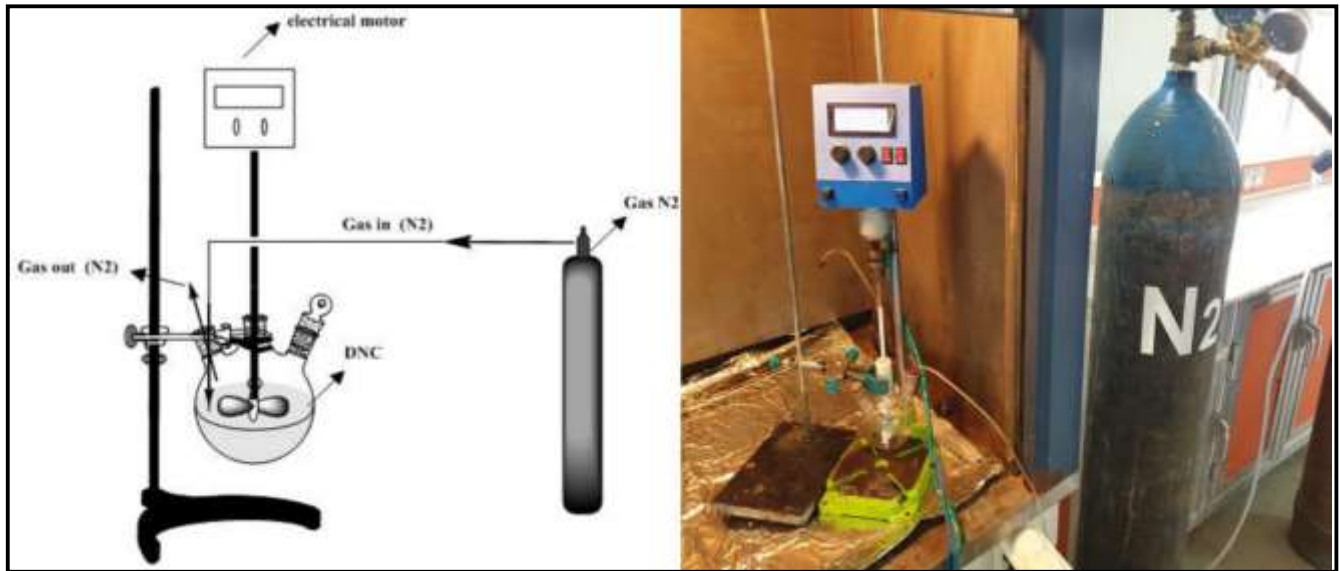


Figure 1: Schematic presentation and experimental of mixing system.

2.2. Methods

According to the wear test standard described in ASTM D5963-97a, the specimen has a diameter of 1 mm and a length of 2 mm [17]. Wear testing was performed on an open rotating by testing machine Pin -on- Disc. The mass loss of the tested specimens was measured by weighing way, which is the simplest method of determining the wear rate of the tested specimens. After cleaning the specimens, they were weighed by electrical balance before and after the testing process, the resultant loss in weight was applied in the formulas below to determine the rate of wear. A load of the test was a variable load in the range of (1.5 N - 6 N) and the speed and time of sliding were within the range of (0.5 m/sec. - 3.05 m/sec.), (300 sec.), respectively. The wear rate was estimated as follows [18]:

$$Kc = \frac{Vr}{X} \text{ Where } Vr = \frac{\Delta m}{Pc} \quad X = Vs \times T$$

$$Kc = \frac{\Delta m}{Pc \times Vs \times T} = \frac{m1 - m2}{Pc \times Vs \times T} \quad (1)$$

Where, Kc is the wear rate of composite (mm^3/mm), Δm : Mass loss (g), $m1$ and $m2$ are weights of the specimen before and after the test respectively (g), ρ_c is the density of specimen (g/mm^3), VS is the sliding Speed (mm/s)

and T is the sliding Time (s). The hardness measurement was done according to (ASTM D 2240) by using shore hardness (D) and at room temperature. Each sample was tested in diverse places of it (7 times) at the same time, then takes the average of these values; all tests were done at room temperature [19]. The surface roughness test was carried out by the profilometer device (TR200-type). The measurement was done by fixing the specimens on the surface of the machine, applying the needle of the device perpendicular to the specimen, after moving the needle linearly along the measured length, the readings have been taken three times on different positions on the surface of the specimen and then the average value was determined.

3. Results and Discussion

3.1. Selecting the best Ratio of Nano-fillers Content

The amount of filler in the composite material is a critical element in controlling the physical and mechanical properties of the material. To find a better ratio of nano-fillers in composites that gives a significant enhancement in the mechanical properties of resins used in dental applications. Two types of matrix monomers groups of the prepared copolymers (D and E) were chosen to be reinforced with different ratios of nanoparticle content of hydroxyapatite which are 1, 2, 3, and 4 %wt. The relationship between the filler content of (nHA) particles in resins and the wear resistance, hardness, and surface roughness of the specimens for both groups are presented in Figures 2, 3, and 4, respectively.

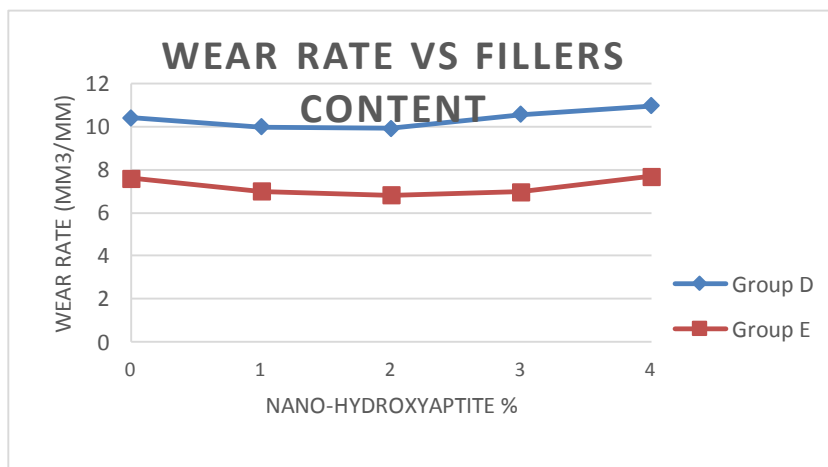


Figure 2: Wear rate for hybrid nanocomposites groups (D and E) as a function of filler content (nano-hydroxyapatite) in the composite.

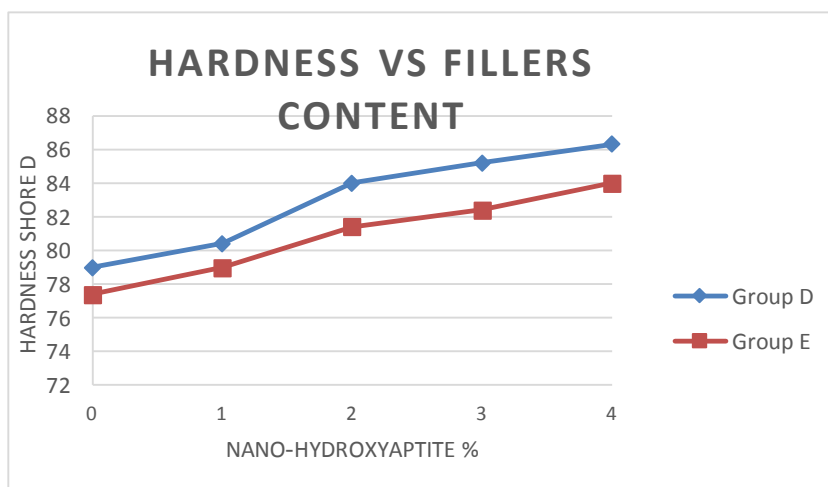


Figure 3: Hardness for hybrid nanocomposites groups (D and E) as a function of filler content (nano-hydroxyapatite) in the composite.

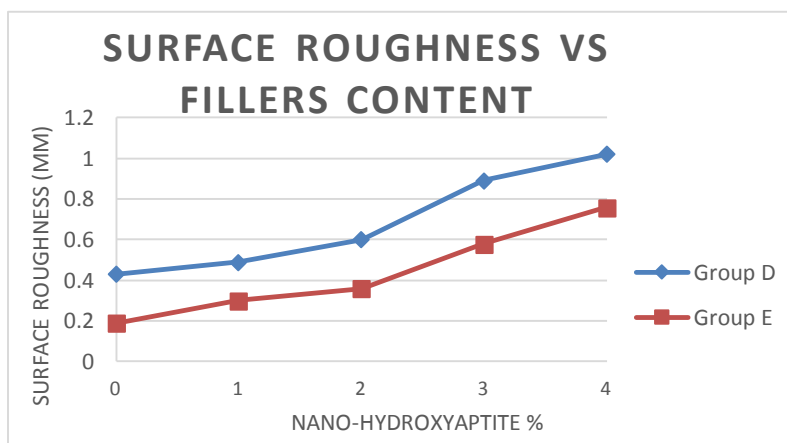


Figure 4: Surface roughness for hybrid nanocomposites groups (D and E) as a function of filler content (nano-hydroxyapatite) in the composite.

It can be noticed that the values of hardness and surface roughness properties were slightly increased with the addition of (1 wt%) of nHA for both groups of resin, these values continuously increased with increasing of the weight of (nHA) particles and can observe the maximum value of hardness (86.3 for D and 84 for E) and surface roughness ($1.02\mu\text{m}$ for D and $0.76\mu\text{m}$ for E) were at (4 wt%) of hydroxyapatite. This is due to the previously reported improvement of the mechanical properties that are associated with the increasing content of fillers particles and is related to the high hardness and brittleness that have these particles as compared with the resin matrix. The wear rate has been reduced by adding the (1wt %) of nHA for groups D and E of resin to reach the lowest value at 2wt% before its jumping to the highest value at 4wt% of nHA. In the 4wt % nanofiller ratio, these properties are significantly increased compared to the control specimens; however, the increase of wear rate and surface roughness is not desirable. Therefore, it can be concluded in this study that the best filler content must be used to achieve the high development in all mechanical properties of copolymers is exactly 2wt%.

3.2. Mechanical Test of the Nanocomposites

From the result wear rate shown in Table 1 and results in Figure 5, it was found that all copolymers (free from fillers) without fillers recorded significantly higher mean weight loss values than the nanocomposites mean values. It was observed that the tested composites, reinforced with different powders of nanoparticles, exhibited different wear rates. These results are in good agreement with other previous studies [17], which explained that these different wear rates may be attributed to the difference in material properties. Particles type, volume by weight, and distribution play a major role to keep the stability of the materials [20, 21]. In addition to the filler system, the filler–matrix coupling also has a significant power on the value of composites wear [22]. From Figure 5 it was found that the value of wear rate was decreased as the nanofillers are added; the lowest value ($6.11\text{mm}^3/\text{mm}$) was noticed at the group (E) of copolymer matrix nanocomposite that contains on SiO_2 nanoparticle. While the higher values were for nanocomposite that contains nano-Zirconia with the group (C) of copolymer matrix. The fact that silica particles are harder than the other filler as mentioned before that during testing responded about the high wears resistance of composites contains it. This means that the polymer reinforced with SiO_2 fillers has decreased the wear rate (increase abrasion wear resistance) higher than HA, ZrO_2 , and Al_2O_3 fillers. And this depends on the compatibility between the components of the matrix material and the inorganic nano reinforcement materials. Moreover, one of the most important factors that affect the abrasions wear resistance is the interfacial properties, it depends on the extent of bonding at the reinforcing interface between the nanoparticles and the matrix material. The larger the contact area, the greater the reinforcement ratio, and this is inversely proportional to the size of the reinforcement particles. Many researchers have mentioned that silica-filled composite has been recommended instead of other filler of composite [23]. This is because of the reinforcement, which is decreased because of a breakdown at the interface of matrix reinforcement or failure in the reinforcement itself. Finally, the mechanical properties of the SiO_2 ceramic fillers are harder than others in nature [24].

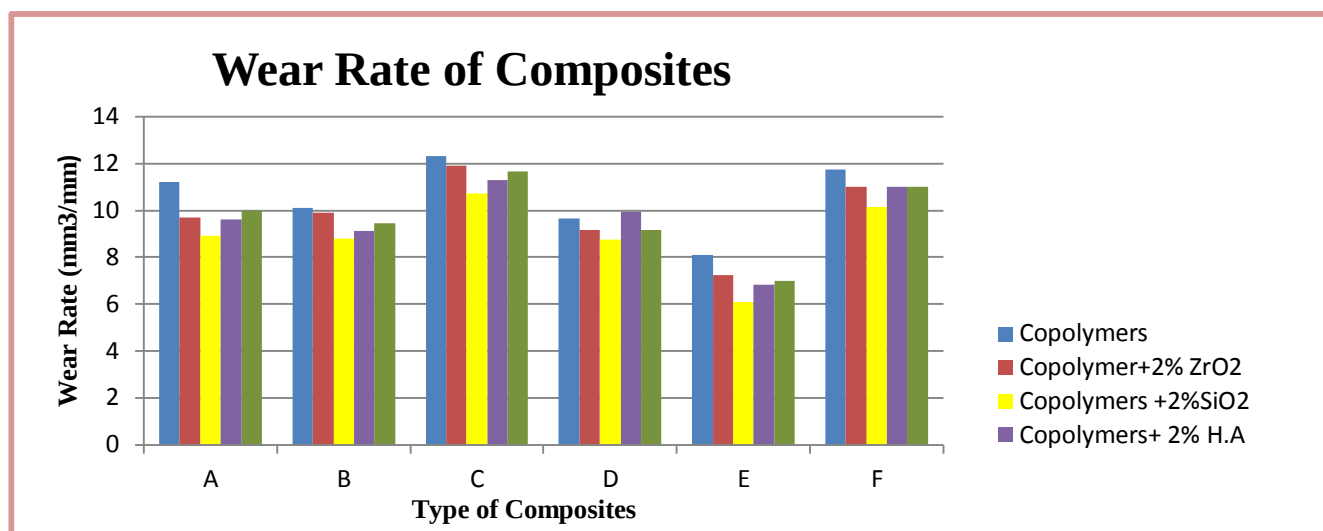


Figure 5: Wear rate of prepared composite as a function of filler type and the type of polymer blends for the matrix material.

The result of the hardness test in Figure 6 shows an increment of the hardness with the addition (2%wt) ratio of nanoparticles (ZrO₂, SiO₂, HA and Al₂O₃) individually in the copolymer matrix materials. The increment in hardness values is dependent on the type of both fillers and polymeric materials; the highest value of hardness was reached to (85) that seen at nanocomposite which based on copolymers of group D and reinforced by SiO₂ nanoparticle. While the lowest values were for nanocomposites that were based on copolymers of the group (A) and reinforced by Zirconia nanoparticles, as well, was noticed from Figure 6 that hydroxyapatite nanofillers had the maximum value of improvement of two groups (A and C) nanocomposites. This high hardness value of the composites was due to that the existence of particles of filler in resin matrix led to decreasing the movement of polymer chains molecular and destruction of the mobility of the dental composite matrix, especially by the addition of the filler content in nano size, this may be related to the high surface area of fillers which in contact with dental composite material and attribute to increasing the hardness [25, 26].

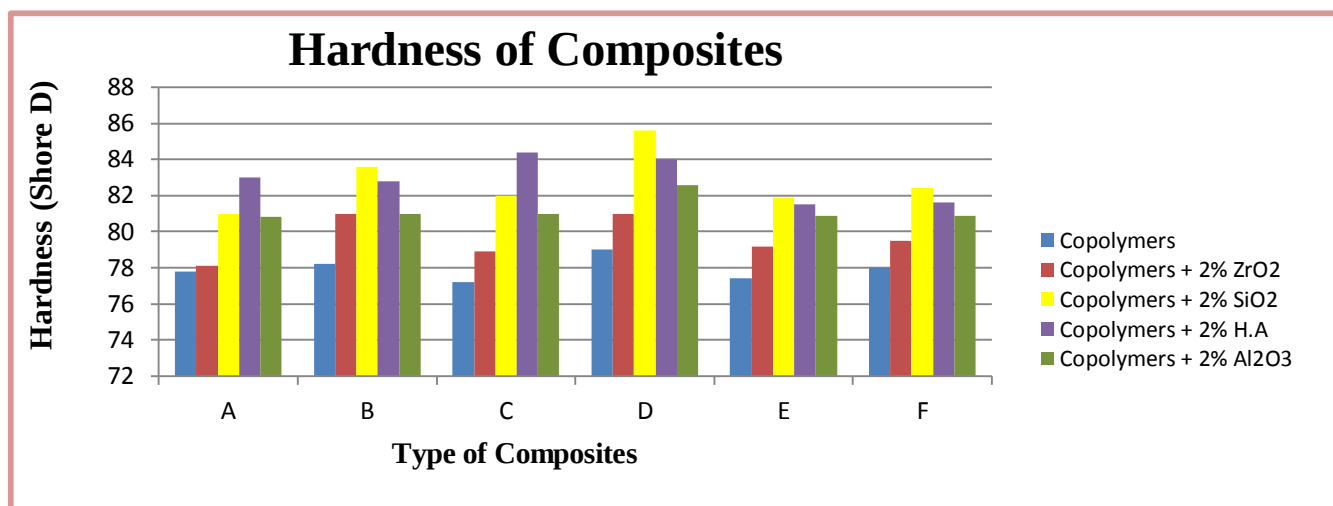


Figure 6: Hardness of prepared composite as a function of fillers type and the type of polymer blends for matrix material.

The difference in hardness values is also clearly observed in this figure that may be certified to the difference in both organic matrices of copolymers and filler types. The chemical composition of monomer content has an important effect on the mechanical properties of resin composites. Therefore, for the same types of filler, some monomers which participate in the composition of copolymers matrices of composite resin have been caused a

considerable enhancement in mechanical properties and led to an increase in values of hardness. Also enhances the hardness values of composites, the uniform dispersion of fillers, as well as, strong interfacial adhesion between resin/fillers must be existing [17]. Fillers are imparting the restorative materials with sufficient strength and hardness to resist the stresses and strains of the oral cavity and reach acceptable clinical longevity [28]. Other factors that affect the hardness of composite material are the nature, volume fraction, and size of the filler, as well as, the interfacial adhesion between the composite components and inorganic nanofiller, and the surface finishing [29]. The size of the filler has an impact on composite hardness, where dental composites that have been reinforced with Nanoparticles have shown high values of hardness over that free from nanofiller. Nanoparticles have a considerable increase in dental composite hardness, which have been reinforced and all used fillers were with nano size and have a dissimilar effect on the composite hardness that connected to filler type. Next, it should be noted that in the current work the highest hardness was obtained with both silica and hydroxyapatite fillers. This can be attributed to the degree of compatibility between each one of these nano-fillers and the components of the matrix material. Besides the filler content in the prepared composite which is constant in this study, and the size of particles, several factors considerably increase dental composite hardness, like: 1) Fundamental characteristics of some of the particles of the filler, like HA, SiO₂, and ZrO₂. Those particles show strong ionic interatomic bonding for conferring desirable characteristics, like a high level of hardness [30], 2) The regular Nano-particles dispersion gives a sufficient distance amongst particles, which increases the hardness and reinforcement of the composites, 3) Strong interfacial interaction between the inserted Nano-particles and polymer, and 4) Properties of filler particles that are harder show a higher level of hardness of the surface in the composites [31]. A smooth surface is important to continue on dental restorations to avoid many problems such as discoloration and change in brightness as well as to minimize the risk of secondary caries. The formation of bacterial plaque was encouraged rough surfaces, which can be harmful to periodontal health. To achieve the best clinical results, it is important to keep the composite resin surface as smooth as possible [32]. The mean surface roughness (Ra, μm) values for the composite resins are shown in Figure 7, this figure indicates that the reinforcing of matrixes with nanoparticles leads to a clear increase in surface roughness. Groups A and F showed the highest roughness values of (0.82 & 0.79) μm respectively. Groups B and D had significantly fewer roughness values (0.16 & 0.19) μm than all other groups, which created the smoother surfaces among all used resin. It was also found that the highest surface roughness was obtained with the specimen containing (ZrO₂) fillers rather than the specimen containing other used fillers (SiO₂, Al₂O₃) while the lowest value was found in composites with HA fillers.

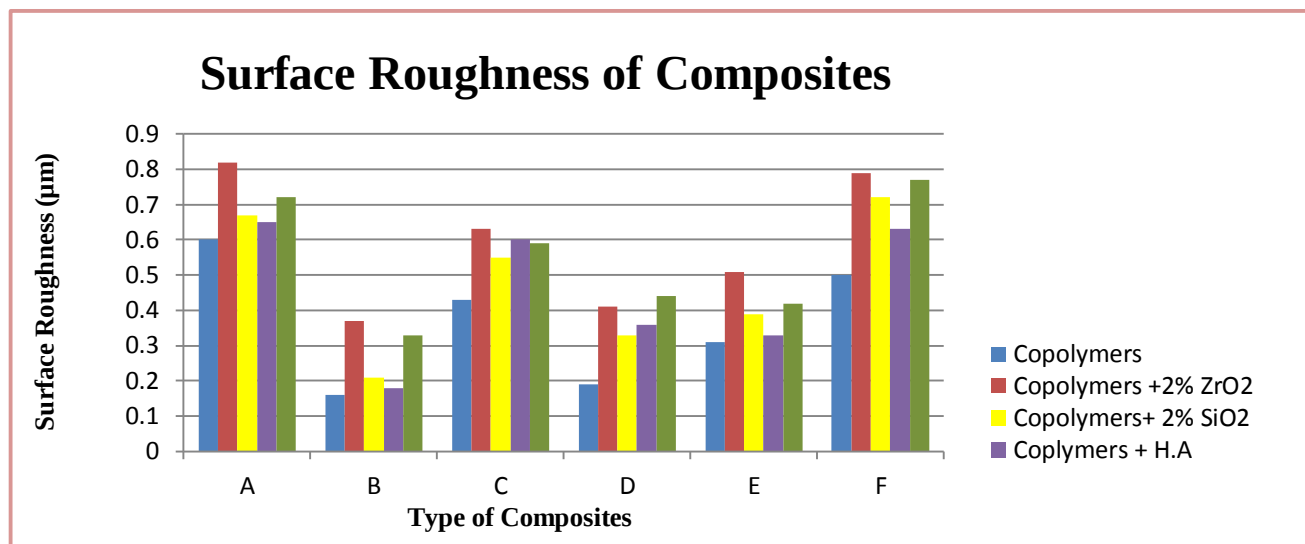


Figure 7: Surface roughness of prepared composite as a function of filler type and the type of polymer blends for matrix material.

Many factors have more effect on the surface roughness property, the interaction of these factors is related to composite composition, such as type, size, shape, and distribution of fillers, in addition to the type of resin matrix, the bond efficiency at the filler/matrix interface and the degree of final cure achieved, [33]. It has been important

to note that restoration with a Ra value of fewer than 1 μm seems to be smooth [34]. Thus, all produced resin composites in this study have optically satisfactory Ra values.

4. Conclusions

The following conclusions were obtained as a result of this study: 1) Successfully using the photopolymerization process to fabricate new dental restorative nanocomposites more than that present in markets including unique monomers and different fillers. 2) The test results showed the wear rate, hardness, and roughness values differed depending on the chemical composition of the matrix components and the kinds of inorganic nanofiller. 3) The nanocomposite that is built on a copolymer of group E containing (methacrylamide and meth acrylic acid monomers) and reinforced by silica nanoparticles showed the highest values in wear resistance ($6.11\text{mm}^3/\text{mm}$). So, it can be the most promising material in dental restoration. 4) The highest value of hardness was (85) was nanocomposite which is based on copolymers of group D and reinforced by SiO_2 nanoparticles. 5) Nanocomposite that is based on a copolymer of groups B and D have surface roughness (0.16 & 0.19) μm values, which shows better surface roughness properties making it a more clinically suitable option for dental restorative materials.

Acknowledgement

The authors express their sincere appreciation to the Applied Science Department University of Technology- Iraq.

Conflict of Interest

There are no conflicts of interest regarding the publication of this manuscript.

References

- [1] P. Suwannaroop, P. Chaijareenont, and N. Koottathape "In Vitro Wear Resistance, Hardness and Elastic Modulus of Artificial Denture Teeth" *Dent Mater J*; 30: 461–468, 2011.
- [2] A. M. Al-Kinani, A.J. Haider., and Sh. Al-Musawi, "Design, Construction and Characterization of Intelligence Polymer Coated Core–Shell Nanocarrier for Curcumin Drug Encapsulation and Delivery in Lung Cancer Therapy Purposes" *Journal of Inorganic and Organometallic Polymers and Materials*, ISSN 1574-1443, 2020. <https://doi.org/10.1007/s10904-020-01672-w>
- [3] A. A. Atiyah, A.J. Haider, and R.M. Dhahi "Cytotoxicity Properties of Functionalised Carbon Nanotubes on Pathogenic Bacteria". *IET Nanobiotechnology* 13:597–601, 2019 <https://doi.org/10.1049/iet-nbt.2018.5394>
- [4] A. D Thamir, A. J. Haider, F. Q. Mohammed, and Kh. M. Chahrour "Hybrid Gas Phase Ti-BCN Coatings Doped with Al" *Journal of Alloys and Compounds*, vol. 723, pp. 368-375, 2017.
- [5] S. R. Braga, T. Y. Tachibana, N. Garone-Netto et al. "Abrasion resistance of different composites". *J Health Sci Inst*; 29: 85–88, 2010.
- [6] S. Hahnel, M. Behr, and G. Handel " Two-body Wear of Artificial Acrylic and Composite Resin Teeth in Relation to Antagonist Material" *J Prosthet Dent*; 101: 269–278, 2009.
- [7] R. D. Paravina, L. Roeder, H. Lui, K. Vogel, and J.M Powers "Effect of Finishing and Polishing Procedures for the Surface Roughness, Brightness and Color of the Resin Based Composites". *J Am Dent*.17:262-66, 2004.
- [8] S.C. Bayne. Dental composites/glass ionomers: Clinical reports. *Adv Dent Res*. 6: 65-77, 1992.
- [9] C. P. Turssi, D. M. Purquerio, and M.C. Serra "Wear of dental resin composites: Insights into underlying processes and assessment methods – A review". *J Biomed Mater Res B*. 65: 280–85, 2003.
- [10] K.j. Soderholm, and N. D Richards "Wear Resistance of Composites: A Solved Problem" *Gen Dent*. 46: 256-65, 1998.

- [11] C. P. Turssi, J.L. Ferracane, and Vogel K. "Filler Feature and their Effects on Wear and Degree of Conversion of Particulate Dental Resin Composites". *Biomaterials* 26: 4932-37, 2005.
- [12] L.H. Mair, T.A. Stolarski, R.W. Vowles, and L.CH. Ioyd. "Wear: Mechanisms, Manifestations and Measurement". *Report of a Workshop. J Dent* 24:141–148, 1996.
- [13] V.V. Badra, J.J Faraoni, R.P. Ramos, and R.G. Palma-Dibb "Influence of Different Beverages on the Microhardness and Surface Roughness of Resin Composites". *Oper Dent* 30: 213-219, 2005.
- [14] C. Zanter, A.M. Kielbassa, P. Martus, and K.H. Kunzelmann "Sliding Wear of 19 Commercially Available Composites and Compomer". *Dent Mater* 20:277–285, 2004.
- [15] K. Handa, N. Murakami, T.Yamazaki, H. Takahashi, and N Wakabayashi. "The Ball-on-Disk Cyclic Wear of CAD/CAM Machinable Dental Composite and Ceramic Materials". *J Oral Sci.* 59: 589-96, 2017.
- [16] C. Bencang, S. Fengbo, D. Qian, W. Huining, L. Yuanhua, S. Yang, and L. Ming "Preparation and Characterization of Sodium Aluminum Silicate-Polymer Composites and Effects of Surface Roughness and Scratch Directions on Their Flexural Strengths" *ORIGINAL RESEARCH* April 2021 Volume 8 | Article 655156 doi: 10.3389/fmats. 655156. 2021
- [17] Standard Test Method for Rubber Property-Abrasion Resistance D 2228, Annual Book of ASTM Standard, Vol 09.01, USA, 1988.
- [18] D. Dowson, "The History of Tribology", 2nd edition, MEP, Longman, London, 1998.
- [19] "Standard Test Method for Plastics Properties- Durometer Hardness D 2240", Annual Book of ASTM Standard, Vol. 09.01, 1988.
- [20] O. Mohamed and I. Sakr "Evaluation of Wear Resistance of Opposed Recent Types of Dental Composites" *International Journal of Medicine in Developing Countries* 2(1):21–26, 2018.
- [21] I. Ghazi, S. Salih, J. Oleiwi, and M. Mutar "Evaluation of Diametral Tensile and Compressive Strengths of Different Types of Nanocomposites for Dental Applications" *Materials Today: Proceedings* 49 2641–264, 2022.
- [22] O. Savabi, F. Nejatidanesh, M. F. Hossein, A. Arsalan, and G. Savabi "Evaluation of Hardness and Wear Resistance of Interim Restorative Materials" *Dental Research Journal* Vol 10, Issue 2, 2013.
- [23] A. Magdalena, W. Arie, P. Jolanta, J. M. Franciscus, J. Cornelis, and B Kleverlaan. "Contact- and Contact-free Wear Between Various Resin Composites". *Dent Mater J* 31:134–40. <https://doi.org/10.1016/j.dental.2014.11.007>, 2015.
- [24] G.Y. Lee, C.K.Dharan, and R.O. Ritchie, "A Physically-Based Abrasive Wear Model for Composite Materials", Depart. Of Materials Science and Engineering, University of California, 2007.
- [25] M. A. Mutar, I. F. Ghazi, and M.S. Mahdi "Preparation and Characterization of Novel Bis- GMA Dental Nanocomposite and their application as dental material: Mechanical Properties and Water Sorption/Volumetric Shrinkage" *Materials Science and Engineering* vol 870: 012051, 2020.
- [26] R.H. Hussein, A.A. Taha, and O. M. Abdulhusein "Study of Biological Activities of Magnetic Iron Oxide Nanoparticles Prepared by Co-Precipitation Method" *Journal of Applied Sciences and Nanotechnology*, Vol. 1, No. 2 2021.
- [27] S.Sava, M. Moldovan, C Sarosi, A. Mesarosi, D. Dudeai, and C. Alb "Effects of Graphene Addition on the Mechanical Properties of Composites for Dental Restoration" *MATERIALE PLASTICE* 52 , No. 1 , 2015.

- [28] K.S. Parag "Role of Filler and Functional Group Conversion in the Evolution of Properties in Polymeric Dental Restoratives" *Dental Material*. 30(5): 586–593, 2014.
- [29] F. Kundie, C. Husna Azhari, A. Muchtar and Z. A. Ahmad "Effects of Filler Size on the Mechanical Properties of Polymer-filled Dental Composites: A Review of Recent Developments" *Journal of Physical Science*, Vol. 29(1), 141–165, 2018.
- [30] M. Lyapina "Application of Nanobiomaterials in Restorative Dentistry". J. IMAB, 22(1), 1050–1055, 2016.
- [31] P. Vallittu "Non-metallic Biomaterials for Tooth Repair and Replacement" *Cambridge Woodhead Publishing*.
- [32] H. A. Sharhan, Z. N. Rasheed, and J. K. Oleiwi "Synthesis and Physical Characterization of PMMA/PP and PMMA/ PAN Composites for Denture Application" *Journal of Applied Sciences and Nanotechnology*, Volume 1, Issue 3, Pages 13-23, 2021, 10.53293/jasn.2021.3759.1040
- [33] B. Buchgraber, L. Kqiku, N. Allmer, G. Jakopic, and P. Städtler, "Surface Roughness of One Nanofill and One Silorane Composite After Polishing" *Collegium Antropologicum*, vol. 35, no. 3, pp. 879-883, 2011. Chung KH: "Effects of Finishing and Polishing Procedures on the Surface Texture of Resin Composites" *Dent Mater*. 10:325-30. 10.1016/0109-5641(94)90041-8, 1994.